

Model	Spectrophotometer CM-5	
Illumination/viewing system	Reflectance:	di:8°, de:8° (diffuse illumination: 8° viewing) SCI (specular component included)/SCE (specular component excluded) switchable Conforms to CIE No. 15, ISO 7724/1, ASTM E 1164, DIN 5033 Teil 7, and JIS Z 8722 (Condition c)
	Transmittance:	di:0°, de:0° (diffuse illumination: 0° viewing)
Integrating sphere size	Ø152 mm	
Detector	Dual 40-element silicon photodiode arrays	
Spectral separation device	Planar diffraction grating	
Wavelength range	360 nm to 740 nm	
Wavelength pitch	10 nm	
Half bandwidth	Approx. 10 nm	
Measurement range	0 to 175 % (Reflectance or transmittance); Output/display resolution: 0.01%	
Light source	Pulsed xenon lamp	
Measurement time	Approx. 1 s (to data display/output); Minimum measurement interval: Approx. 3 s	
Measurement/ illumination area	Reflectance:	Changeable by changing mask and settings. LAV: Ø30 mm/Ø36 mm; MAV (optional): Ø8 mm/Ø11 mm; SAV (optional): Ø3 mm/Ø6 mm
	Transmittance:	Ø20 mm
Repeatability	Spectral reflectance: Standard deviation within 0.1% (400 nm to 740 nm) Chromaticity value: Standard deviation within ΔE*ab 0.04 * When a white calibration plate is measured 30 times at 10-second intervals after white calibration	
Inter-instrument agreement	Within ΔE*ab 0.15 (Typical) (LAV/SCI) (Based on 12 BCRA Series II color tiles compared to values measured with a master body under Konica Minolta standard conditions)	
Transmittance chamber	No sides (unlimited sample length); Depth (maximum sample thickness): 60 mm Sample holders (optional) for holding sheet samples or containers of liquid samples can be installed/removed	
Display	5.7-inch TFT color LCD	
Display languages	English, Japanese, German, French, Italian, Spanish, Simplified Chinese	
White/100% calibration	Automatic white (reflectance)/100% (transmittance) calibration using internal white calibration plate (Not applicable to 100% calibration when using cells for transmittance measurements of liquids.)	
Interfaces	USB 1.1 (Connection to PC; USB memory stick); RS-232C standard (Connection to serial printer)	
Observer	2° Standard Observer or 10° Standard Observer	
Illuminant	A, C, D50, D65, F2, F6, F7, F8, F10, F11, F12, ID50, ID65 (simultaneous evaluation with two light sources possible)	
Displayed data	Spectral values, spectral graph, colorimetric values, color-difference values, color-difference graph, pass/fail judgment, pseudo color, color assessment	
Color space	L*a*b*, L*C*h, Hunter Lab, Yxy, XYZ, Munsell, and color differences in these spaces (except for Munsell)	
Index	Reflectance:	MI; WI (ASTM E 313-73, ASTM E 313-96); YI (ASTM E 313-73, ASTM E 313-96, ASTM D 1925); ISO Brightness; B (ASTM E 313-73)
	Transmittance:	Gardner; Iodine Color Number; Hazen/APHA; European Pharmacopoeia; US Pharmacopeia
User index	User-defined index	
Color-difference equation	ΔE*ab (CIE 1976), ΔE*94 (CIE 1994), ΔE00 (CIE 2000), ΔE (Hunter), CMC (l: c)	
Pass/fail judgment	Tolerances can be set to colorimetric values (except Munsell), color-difference values, or reflectance index values	
Storable data	Measurement data: 4,000 measurements; Target color data: 1,000 measurements	
USB memory stick* storage	Storage of measurement data and target color data. Storage/reading of measurement condition settings	
Power	AC 100 to 240 V, 50/60 Hz (using exclusive AC adapter)	
Size	Slide cover closed: 385 (W) × 192 (H) × 261 (D) mm Slide cover open: 475 (W) × 192 (H) × 261 (D) mm	
Weight	Approx. 5.8 kg	
Operating temperature/ humidity range	13 to 33°C, relative humidity 80 % or less (at 35°C) with no condensation	
Storage temperature/ humidity range	0 to 40°C, relative humidity 80 % or less (at 35°C) with no condensation	

SAFETY PRECAUTIONS

For correct use and for your safety, be sure to read the instruction manual before using the instrument.

- Always connect the instrument to the specified power supply voltage. Improper connection may cause a fire or electric shock.
- Be sure to use the specified batteries. Using improper batteries may cause a fire or electric shock.




Certificate No : YKA 0937154
 Registration Date : March 3, 1995

Certificate No : JQA-E-80027
 Registration Date : March 12, 1997

Phone : +31(0)30 248-1193	Fax : +31(0)30 248-1280
Phone : +49(0)89 4357 156 0	Fax : +49(0)89 4357 156 99
Phone : +33(0)1 4937-82519	Fax : +33(0)1 4937-84771
Phone : +44(0)1908 540-622	Fax : +44(0)1908 540-629
Phone : +39 02 39011.1	Fax : +39 02 39011.223
Phone : +32 (0)2 7170 971	Fax : +32 (0)2 7170 977
Phone : +41(0)43 322-9800	Fax : +41(0)43 322-9809
Phone : +46(0)31 7099464	Fax : +46(0)31 474945
Phone : +43(0)1 87882-430	Fax : +43(0)1 87882-431
Phone : +48(0)71 33050-01	Fax : +48(0)71 734 52 10
Phone : +86-021-5489 0202	Fax : +86-021-5489 0005
Phone : +86-010-8522 1551	Fax : +86-010-8522 1241
Phone : +86-020-3826 4220	Fax : +86-020-3826 4223
Phone : +86-023-6773 4988	Fax : +86-023-6773 4779
Phone : +86-0532-8079 1871	Fax : +86-0532-8079 1873
Phone : +65 6563-5533	Fax : +65 6560-9721
Phone : +82(0)2-523-9726	Fax : +82(0)2-523-9729

9242-4858-10 AJMAPK① Printed in Japan

Measurements as simple as 1-2-3!



Switch on power.

The CM-5 starts up and **automatically performs white/100% calibration*** using an internal white calibration plate behind the shutter.

* Not applicable to liquid transmittance measurements using cells.



Position sample.


For reflectance, the **top port** makes measuring samples of various shapes and sizes easy. For transmittance, sliding open the CM-5 reveals a **large transmittance chamber**. Liquids can be measured using optional cells.



Press MEAS.


The measurement is taken and the results appear in the display. The **large color LCD** enables data to be shown not only numerically, but also on the colorimetric plots and spectral graphs that normally require a computer to display.

Actual CM-5 screens!

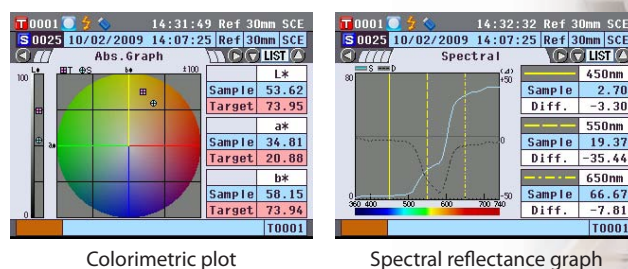

Screens can be shown in any of **7 languages**: English, Japanese, German, French, Italian, Spanish, and Simplified Chinese

Just follow the wizard!

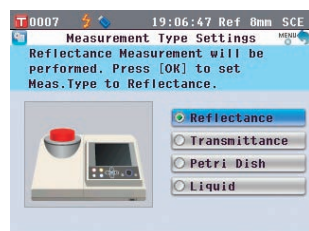

Even beginners can take measurements easily without mistakes.



The CM-5's **wizard mode** guides users through each step, helping users to make settings and take measurements without having to get out the instruction manual each time.

Avoid multi-user confusion with USB!

Do many people in your lab use the same instrument? The CM-5 helps eliminate that confusion by letting users store their own settings on their own USB memory stick, so they can restore the settings they need by simply reading from the memory stick instead of going through and redoing settings individually. Afterwards when they're finished, they can store measurement and target data on the same USB key and take it with them for further analysis.



System Diagram

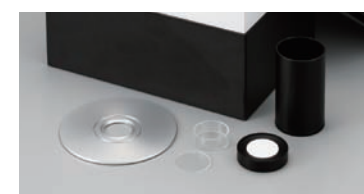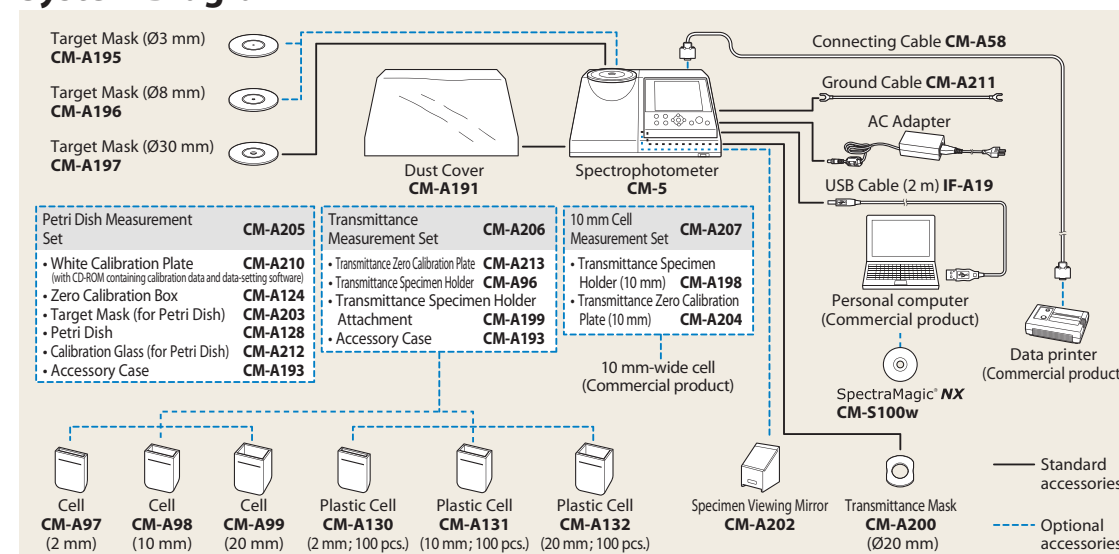

Petri Dish Measurement Set CM-A205



Transmittance Measurement Set CM-A206




10mm Cell Measurement Set CM-A207

Compact, versatile color instrument

Reflectance measurements

The measuring port of the CM-5 is on top, so users can just place a solid object on the port and press the MEAS. button. There's no need to clamp the sample in a sample holder, and there's no worry about the sample shifting position. And, by using a Petri dish (optional accessory), liquids, pastes, and powders can also be measured easily.



Samples are just placed on top, so even large samples can be measured.



By using the Ø3mm target mask (optional accessory), even small samples can be measured.



Chunky materials can be put in a Petri dish (optional accessory) and measured.



Pastes can also be measured using a Petri dish (optional accessory).



Colorant pellets can be measured in raw form using a Petri dish (optional accessory).




Tiny amounts of costly samples can be measured using the mini dish (custom product).

Transmittance measurements

The CM-5's transmittance chamber is large and sideless, enabling measurements of even large sample sheets with thicknesses up to 60mm.

For liquids, optional cells with 3 optical path lengths for different sample densities are available, and commercial 10mm-wide cells can also be used.

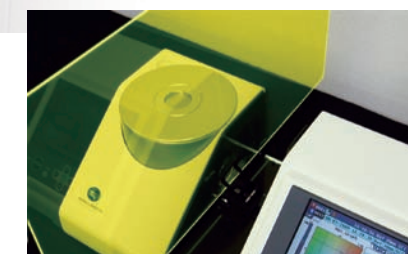

Internal calibration curves for measuring standard chemical/pharmaceutical indices

The CM-5 can measure several of the standard color indices commonly used in the chemical and pharmaceutical field: Gardner, Hazen/APHA, Iodine Color Number, European Pharmacopoeia and US Pharmacopoeia. Calibration curves for these indices are stored in the CM-5, so measurements of samples based on these indices can be performed quickly and easily by anyone.

